


Order Form & Price List


Wheelchair Model _____
 Wheelchair Size (see page 2) _____
 Wheelchair Dropshipped Yes No
 Seat Rail Diameter 7/8" 1"
 Backpost Diameter 3/4" 7/8" 1"
 Upholstery - Contact Surface
 Darlexx Dartex Fabric Rev.Dartex
 Neoprene - Please specify color _____
 Non Contact Surface _____
 Embroidery _____
 Color _____ Print Script

Dealer _____
 PO # _____
 Client Name _____
 Contact Person _____
 Phone # _____
 Fax # _____
 Email _____

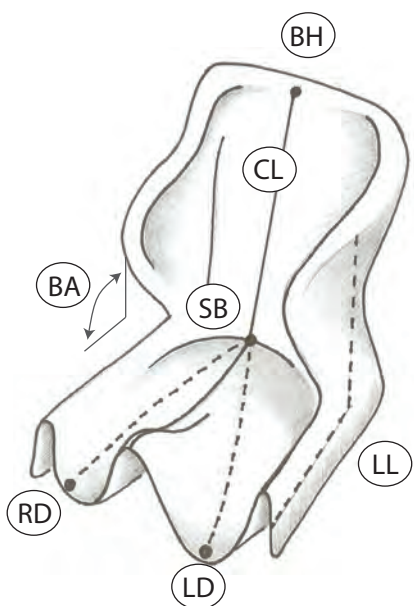

Determine User Contact Width

Centerline of Simulator and Mobility Base (use this as reference point)
 Apparent Centerline - Do NOT Use as Reference Point

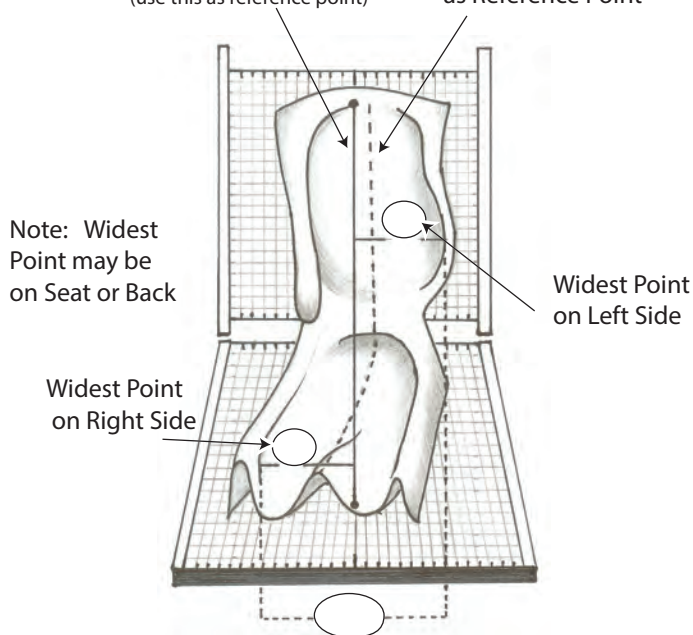

Note: Widest Point may be on Seat or Back

Widest Point on Right Side

Widest Point on Left Side

User Contact Width = Left + Right Widths


Reference Mark Check List

Please Mark the Sample at all Locations

We cannot process without these reference marks

- CL - Centerline - Defines Center of Mobility Base to give proper orientation of Client in Mobility Base
- SB - Seat to Back Reference Line
Determines correct seat depth and back height
- BH - Back Height
- RD - Right Side Seat Depth
- LD - Left Side Seat Depth
- BA - Outside Back to Seat Angle - Reference measurement only
Measured on outside of cast
- LL - Lateral Lines - Must be on both sides. Mark each side same distance from base. Reference line for proper leveling and tilt of system.

Flared Seat and Back - If Total System Width is wider than mobility base, please check for interference with armrest or wheels before ordering this modification



Full System Cut Style

- Taper
- Bucket

